GUIDELINES FOR UPDATE OPERATIONAL STATUS OF EQUIPMENT HOUSING RADIATION SOURCE/SOURCE/RADIATION GENERATING EQUIPMENT (X-RAY DEVICE)


Prior to submission of safety status report, you should update the operational status of all the radiation sources and equipment housing sources, radiation generating equipment (ex. X-ray device) available with you. Otherwise system will not allow you to submit the safety status report.

For Updating Operational Status of RADIATION SOURCE/SOURCE/RADIATION GENERATING EQUIPMENT (X-RAY DEVICE) follow the procedures as mentioned below:


Step-1: Regulatory Forms ----> Common Forms ----> Update Operational Status



Step-2: Following page will be shown after Update Operational Status selection

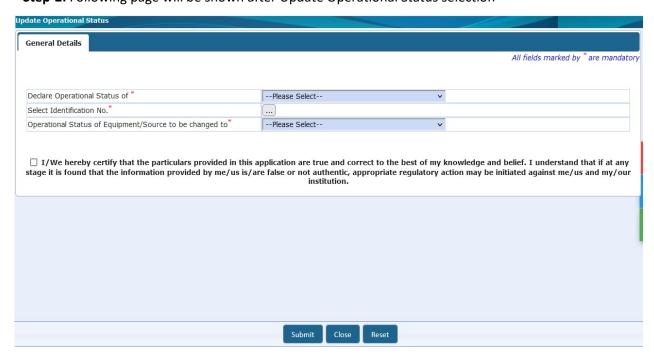


Step-3:

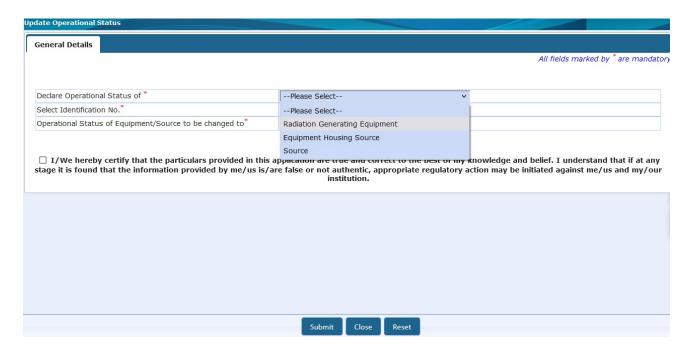


Note: When it is Equipment Housing Source, you have to submit the operational status for both Equipment and source separately

Step-4: Submission of operational status of equipment

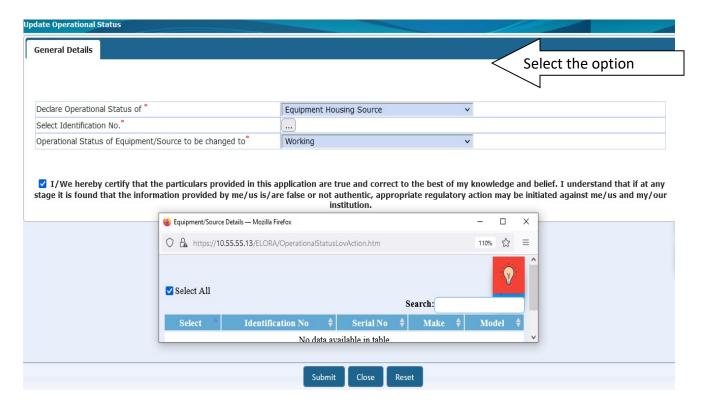

Step-5: Submission of operational status of Source

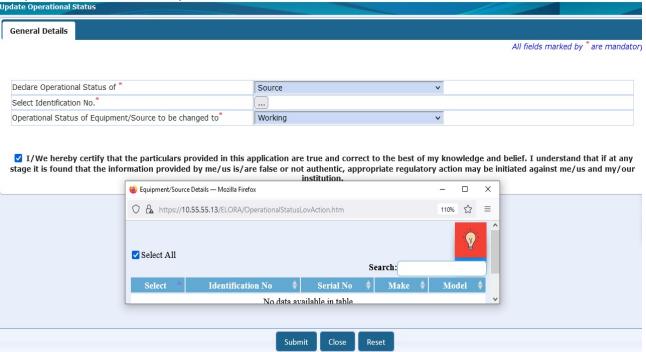

Step-6: Submission of operational status of Radiation Generating Equipment

