


Radiation Warning Symbol

A. For Radioactive Material



B. For X-ray Equipment

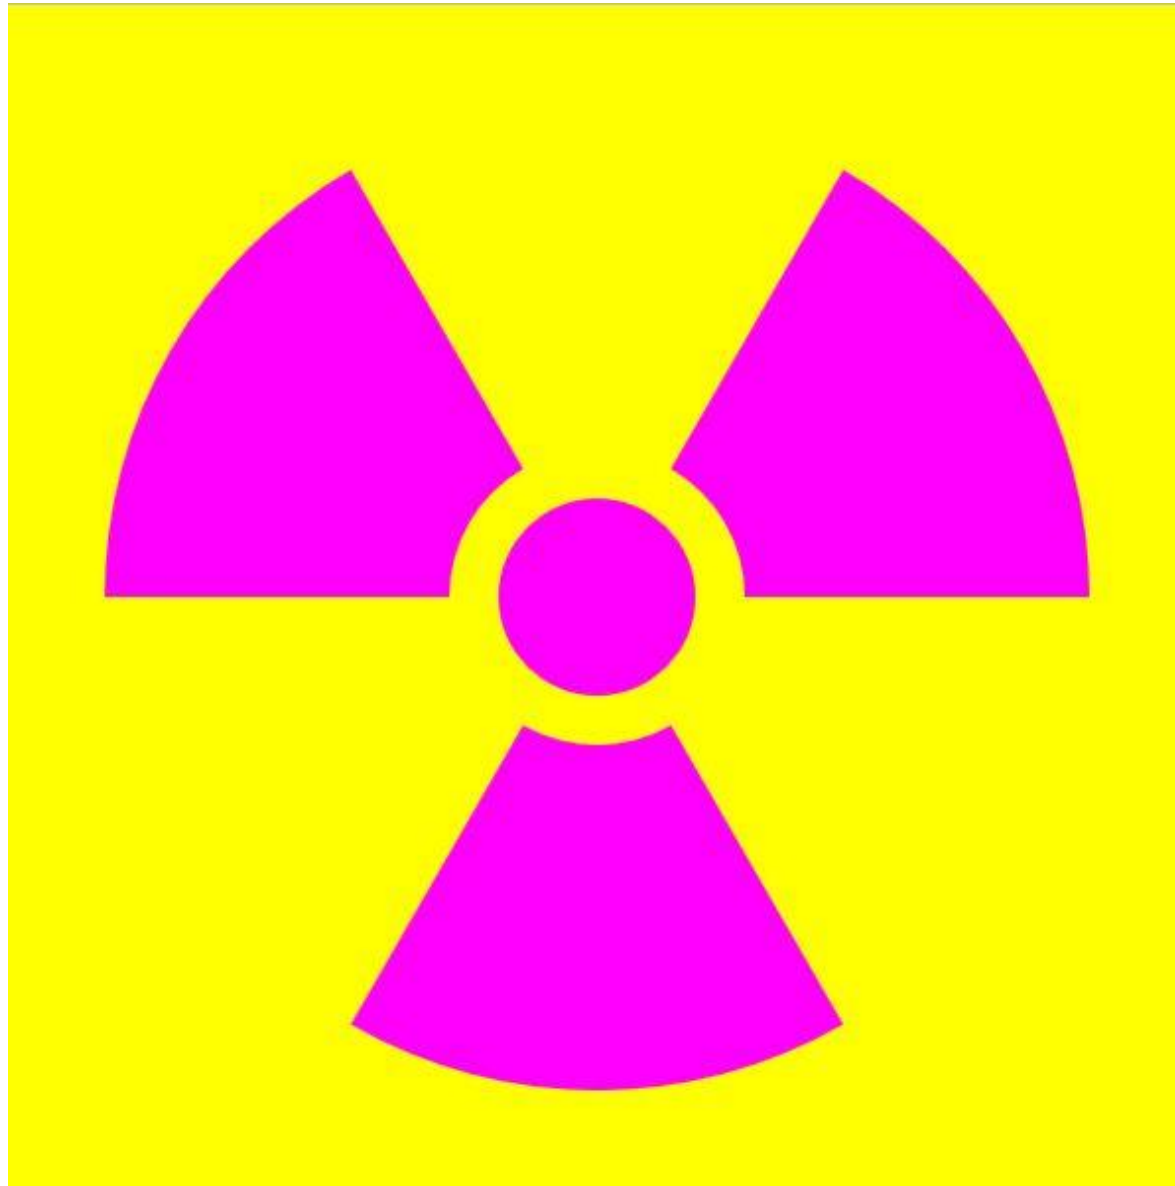

C. Format for warning placard to be pasted outside medical X-ray installation

Type of equipment:
Model Name:
Licence No.



X-RAY EXAMINATION IS GOING
ON INSIDE, DO NOT ENTER

PLEASE WAIT FOR YOUR TURN



CAUTION

IF YOU ARE PREGNANT, OR
THINK YOU MIGHT BE
PREGNANT, TELL THE X-RAY
TECHNOLOGIST BEFORE
HAVING AN X-RAY COMPLETED

DO NOT STAY INSIDE X-RAY
ROOM, IF REQUIRED TO ASSIST
THE PATIENT, INSIST FOR
PROTECTIVE APRON!

Similar display shall be prepared in
local/regional language

Format of warning sign to be
pasted outside medical
diagnostic x-ray installation

PASTE COPY OF AERB LICENCE HERE

To be printed in appropriate size